

GREISINGER electronic GmbH

EASYBus-Sensor module for humidity temperature

with option: selectable humidity display

from version V3.2

Operating Manual

EBHT – 2R / UNI

Content

1	INTENDED USE	2
2	GENERAL ADVICE	2
3	SAFETY INSTRUCTIONS	2
4	DISPOSAL NOTES	2
5	ASSIGNMENT	3
6	DIMENSION	3
7	DISPLAY FUNCTIONS (ONLY AVAILABLE FOR DEVICES WITH OPTION ...-VO)	4
7.1	MEASURING DISPLAY	4
7.2	MIN/MAX VALUE MEMORY	4
7.3	USAGE OF UNIT-LABELS	4
7.4	MIN/MAX ALARM DISPLAY	4
8	ERROR AND SYSTEM MESSAGES	5
9	CONFIGURATION OF THE DEVICE	5
9.1	CONFIGURATION VIA INTERFACE	5
9.2	CONFIGURATION AT THE DEVICE (ONLY AVAILABLE FOR DEVICE WITH OPTION ...-VO)	5
10	NOTES TO THE CALIBRATION SERVICES	7
11	SPECIFICATION	7



WEEE-Reg.-Nr. DE93889386



GREISINGER electronic GmbH
D - 93128 Regenstauf, Hans-Sachs-Straße 26

☎ +49 (0) 9402 / 9383-0 📠 +49 (0) 9402 / 9383-33 📧 info@greisinger.de

1 Intended use

The device measures the relative humidity and temperature of air or non corrosive / non ionizing gases. From this values others can be derived and displayed instead of the rel. humidity.

Field of application

- Room climate monitoring
 - Monitoring of storage rooms
- etc...

The safety instructions (see chapter 3) have to be observed.

The device must not be used for purposes and under conditions for that the device had not been designed. The device must carefully dealt with and has to be used according to the specifications (do not throw, knock, etc.). It has to be protected against dirt.

Do not expose the sensor to aggressive gases (like ammonia) for longer time.

Avoid condensation, as after drying there may remain residues, which may affect the precision negatively.

In dusty environment additional protection has to be applied (special protection caps).

2 General advice

Read through this document attentively and make yourself familiar to the operation of the device before you use it. Keep this document in a ready-to-hand way in order to be able to look up in the case of doubt.

3 Safety instructions

This device has been designed and tested in accordance to the safety regulations for electronic devices. However, its trouble-free operation and reliability cannot be guaranteed unless the standard safety measures and special safety advises given in this manual will be adhered to when using it.

1. Trouble-free operation and reliability of the device can only be guaranteed if it is not subjected to any other climatic conditions than those stated under "Specification".
Transporting the device from a cold to a warm environment condensation may result in a failure of the function. In such a case make sure the device temperature has adjusted to the ambient temperature before trying a new start-up.
2. General instructions and safety regulations for electric, light and heavy current plants, including domestic safety regulations (e.g. VDE), have to be observed.
3. If device is to be connected to other devices (e.g. via PC) the circuitry has to be designed most carefully. Internal connection in third party devices (e.g. connection GND and earth) may result in not-permissible voltages impairing or destroying the device or another device connected.
4. Whenever there may be a risk whatsoever involved in running it, the device has to be switched off immediately and to be marked accordingly to avoid re-starting. Operator safety may be a risk if:
 - there is visible damage to the device
 - the device is not working as specified
 - the device has been stored under unsuitable conditions for a longer timeIn case of doubt, please return device to manufacturer for repair or maintenance.
5. **Warning:** Do not use this product as safety or emergency stop device or in any other application where failure of the product could result in personal injury or material damage.
Failure to comply with these instructions could result in death or serious injury and material damage.

4 Disposal notes




This device must not be disposed as "residual waste".
To dispose this device, please send it directly to us (adequately stamped).
We will dispose it appropriately and environmentally friendly.

5 Assignment

2-wire connection for EASYBus, no polarity, at terminals 1 and 2


6 Dimension

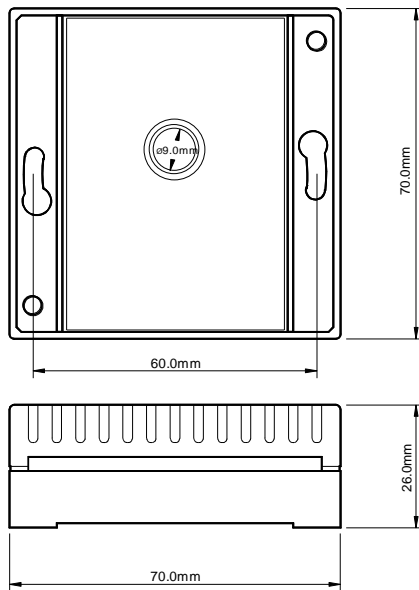


7 Display Functions (only available for devices with option ...-VO)

7.1 Measuring display

During normal operation the **selectable humidity display value** is displayed alternating to the **temperature** in [°C] or [°F].

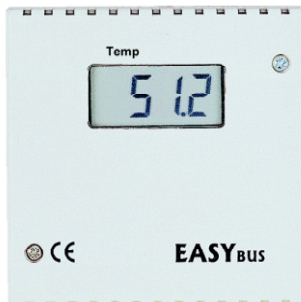

display of selectable humidity value

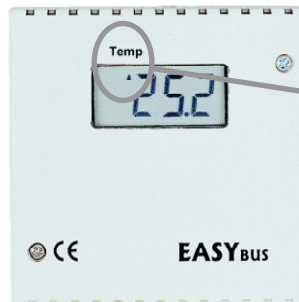

display temperature

Arrow to "Temp" indicates temperature display

If the relative humidity in [%] should be shown, although other display is selected (e.g. dew point temperature, mixing ratio...):

press ▼ (middle key) and ▲ (right key) simultaneous: display changes between 'r.H.' and measurand

7.2 Min/Max Value Memory

Note: the keys will be accessible by removal the cover.

watch Min values (Lo): press ▼ (middle key) shortly once

watch Max values (Hi): press ▲ (right key) shortly once

restore current values: press ▼ or ▲ once again

clear Min-values: press ▼ for 2 seconds

clear Max-values: press ▲ for 2 seconds

display changes between 'Lo' and Min values

display changes between 'Hi' and Max values

current values are displayed

Min values are cleared. Display shows shortly 'CLr'.

Max values are cleared. Display shows shortly 'CLr'.

After 10 seconds the currently measured values will be displayed again.

7.3 Usage of Unit-Labels


As the transmitter is a multiple purpose device, many different display units are possible, e.g. g/kg, g/m³.

Therefore unit-labels (within scope of supply) can be shoved between the case cover and the front foil behind the **transparent unit-window**.

To replace a label, unscrew the cover, pull out the old label (if present) and shove in the new one.

The unit depends on the configuration settings "Unit"!

Please refer to table in chapter "9 Configuration of the device"



7.4 Min/Max Alarm Display

Whenever the measured value is exceeding or undershooting the alarm-values that have been set, the alarm-warning and the measuring value will be displayed alternating.

AL.Lo the lower alarm boundary is reached or is undershot

AL.Hi the upper alarm boundary is reached or is exceeded

8 Error and system messages

Display	Description	Possible fault cause	Remedy
Err.1	Measuring range exceeded	Wrong signal	Temperature above 70°C not allowed.
Err.2	Measuring value below measuring range	Wrong signal	Temperature below -25°C not allowed.
Err.3	Display range has been exceeded	Value >9999	Check settings
Err.7	System fault	Error in device	Disconnect from supply and reconnect. If error remains: return to manufacturer
Err.9	Sensor error	Sensor or cable defective	Check sensors, cable and connections, damages visible?
Er.11	Calculation not possible	Calculation variable missing or invalid	Check temperature
8.8.8.8	Segment test	The transducer performs a display test for 2 seconds after power up. After that it will change to the display of the measuring.	

9 Configuration of the device

9.1 Configuration via interface

The configuration of the device is done by means of the PC-software EASYBus-Configurator or EBxKonfig. The following parameters can be changed:

- Adjusting of humidity and temperature display (offset and scale correction)
- Setting of the alarm function for humidity and temperature

The adjusting by means of offset and scale is intended to be used to compensate errors of the measurements. It is recommended to keep the scale correction deactivated. The display value is given by following formula:

$$value = measured\ value - offset$$

With a scale correction (just for calibration laboratories, etc) the formula changes:


$$value = (measured\ value - offset) * (1 + scale\ adjustment/100)$$

9.2 Configuration at the device (only available for device with option ...-VO)

Note: If EASYBus sensor modules are operated by a data acquisition software, there can be problems if the configuration is changed during a running acquisition. Therefore it is recommended not to change configuration values during a running recording and furthermore to protect it against manipulation by unauthorised persons. (please refer to right picture)

Follow these instructions to configure the functions of the device:

- Press key 1 (**SET**) until the first parameter **Unit** appears in the display
- If a parameter should be changed, press key 2 (**▼**) or key 3 (**▲**), The device changed to the setting – edit with **▼** or **▲**
- Confirm the value with 1 (**SET**).
- Jump to the next parameter with 1 (**SET**).

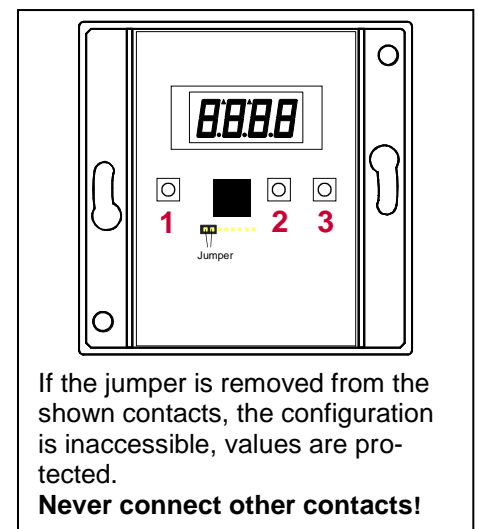

If the jumper is removed from the shown contacts, the configuration is inaccessible, values are protected.

Never connect other contacts!

Parameter	value	information
SET	▼ and ▲	
Unit	Unit and Range of humidity display <i>factory setting: rel.H</i>	
	reL.H	0.0 100.0 % relative air humidity
	F.Abs	0.0 ... 200.0 g/m ³ absolute humidity
	FEU.t	-27.0 ... 60.0°C wet bulb temperature
	t.d.	-40.0 ... 60.0°C dew point temperature
	Enth	-25.0 ... 999.9 kJ/kg Enthalpy
	F.G.	0.0 ... 640.0 g/kg Mixing ratio (atmospheric humidity)
Unit + Temp arrow	Unit of temperature displays <i>factory setting: °C</i>	
	°C	Temperatures in °Celsius
	°F	Temperatures in °Fahrenheit
OFFS	Offset correction of humidity measuring *)	
	oFF	deactivated (<i>factory setting</i>)
	-5.0 ... +5.0	Selectable from -5.0 to +5.0 % rel. humidity
SCAL	Scale correction of humidity measuring *)	
	oFF	deactivated (<i>factory setting</i>)
	-15.00 ... +15.00	Selectable from -15.00 to +15.00 % scale correction
OFFS + Temp arrow	Offset correction of temperature measuring *)	
	oFF	deactivated (<i>factory setting</i>)
	-2.0 ... +2.0	Selectable from -2.0 to +2.0 °C
SCAL + Temp arrow	Scale correction of temperature measuring *)	
	oFF	deactivated (<i>factory setting</i>)
	-5.00 ... +5.00	Selectable from -5.00 to +5.00 % scale correction
ALti	Altitude input (not at all units available) <i>factory setting: 340</i>	
	-500 ... 9000	-500 ... 9000 m selectable
ALLo	Min. alarm-point for humidity measuring	
	-0.1 ... AL.Hi	Selectable from: -0.1 %RH to AL.Hi
ALHi	Max. alarm-point for humidity measuring	
	AL.Lo ... 100.1	Selectable from: AL.Lo to 100.1 %RH
ALdE	Alarm-delay for humidity measuring	
	oFF	deactivated (<i>factory setting</i>)
	1 ... 9999	Selectable from 1 to 9999 sec.
ALLo + Temp arrow	Min. alarm-point for temperature measuring	
	Min.MB ... AL.Hi	Selectable from: min. measuring range to AL.Hi
ALHi + Temp arrow	Max. alarm-point for temperature measuring	
	AL.Lo ... Max.MB	Selectable from: AL.Lo to max. measuring range
ALdE + Temp arrow	Alarm-delay for temperature measuring	
	oFF	deactivated (<i>factory setting</i>)
	1 ... 9999	Selectable from 1 to 9999 sec.

Pressing **SET** again stores the settings, the instruments restarts (segment test)

Please note: *If there is no key pressed within the menu mode within 2 minutes, the configuration will be cancelled, the entered settings are lost!*

*) if higher values are needed, please check sensor, if necessary return to manufacturer for inspection.
Calculation: corrected value = (measured value – Offset) * (1+Scale/100)


10 Notes to the calibration services

Calibration certificates - DKD-certificates - other certificates:

If device should be certificated for its accuracy, it is the best solution to return it with the referring sensors to the manufacturer. (please state desired test values, e.g. 70 %RH)

Only the manufacturer is capable to do efficient recalibration if necessary to get results of highest accuracy! Humidity transmitters are subject to ageing. For optimum measuring precision we recommend a regular adjusting at the manufacturer (e.g. every 2nd year). Cleaning and checking of the sensors is part of the service.

11 Specification

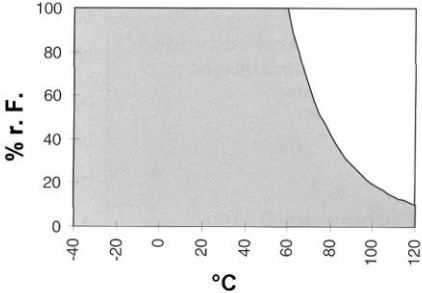Display ranges humidity	Relative air humidity: 0.0...100.0 %RH Wet bulb temperature: -27.0 ... 60.0 °C (or -16,6 ... 140,0 °F) Dew point temperature: -40.0 ... 60.0 °C (or -40,0 ... 140,0 °F) Enthalpy: -25.0 ... 999.9 kJ/kg Mixing ratio (atmospheric humidity): 0.0 ... 640.0 g/kg absolute humidity: 0.0 ... 200.0 g/m ³	
Recommended humidity measuring range	Standard: 20.0 ... 80.0 %RH Option "high humidity": 5.0 ... 95.0 %RH	Working range of humidity sensor: 
Meas. range temperature	-25.0 ... 70.0 °C or -13.0 ... 158.0 °F	
Accuracy Display	(at nom. temperature 25°C) Rel. Air humidity: ±2.5 %RH (<i>within recommended measuring range</i>) Temperature: ±0.4% of meas. value. ±0.3°C	
Media	Non corrosive gasses	
Sensors	capacitive polymer humidity sensor and Pt1000	
Temperature compensation	automatic	
Meas. frequency	1 per second	
Adjusting	Digital offset and scale adjustment for humidity and temperature	
Min-/Max-value memory	Min and max measured values are stored	
Output signal	EASYBus-protocol	
Connection	2-wire EASYBus, polarity free	
Busload	1.5 EASYBus-devices	
Display (only with option VO)	approx. 10 mm high, 4-digit LCD-display	
Operating elements	3 keys	
Ambient conditions		
Nom. temperature	25°C	
Operating temperature	Electronics: -25 ... 70 °C	
Relative humidity	Electronics: 0 ... 95 %RH (not condensing)	
Storage temperature	-25 ... 70 °C	
Housing	ABS (IP65, except sensor head)	
Dimensions	70 x 70 x 28 mm	
Mounting	Holes for wall mounting (in housing - accessible after cover has been removed).	
Mounting distance	60 mm, max. shaft diameter of mounting screws is 4 mm	
Electrical connection	2-pin screw-type terminal, max. wire cross section: 1.5 mm ²	
EMC	The device corresponds to the essential protection ratings established in the Regulations of the Council for the Approximation of Legislation for the member countries regarding electromagnetic compatibility (2004/108/EG). In accordance with EN 61326-1 : 2006, additional errors: <1 % FS. When connecting long leads adequate measures against voltage surges have to be taken.	

